





Federal Office of Public Health FOPH Public Health Directorate Communicable Diseases Division Schwarzenburgstrasse 157 3003 Berne Switzerland

Geneva, April 12, 2022

Geneva Centre for Emerging Viral Diseases

Division of Infectious Diseases

Department of Medicine

Laboratory of virology

Division of Laboratory Medicine

Diagnostic Department

SARS-CoV-2 genomic surveillance in Geneva: weekly update

Highlights:

N/réf: PV/MS

- We continue to observe both a decrease in the number of tests performed at our laboratory and our outpatient center, along with a decrease in the absolute number of positive SARS-CoV-2 tests. The positivity rate however remains high (Figure 1).
- **BA.1** (assessed by the "S Drop out") **is now only rarely retrieved (2.7%), and BA.2 represented more than 97% of the SARS-CoV-2 positive specimens tested** at the end of week 14 (see Figure 2), and the laboratory has stopped systematic S Drop out screening.
- WGS confirmed the replacement of BA.1 by BA.2 (Figure 3; preliminary data, as sequencing is still ongoing for week 13). We continue to observe a **low variability among BA.2 sequences**, with 8% (11/136) carrying the H78Y mutation in the last sequencing batch. No new recombinant has been observed.

Figure 1: Number of SARS-CoV-2 tests performed at the HUG laboratory of virology (per day). Positive tests are displayed in light blue (top). Bottom left: SARS-CoV-2 positive tests over 7 sliding days. Bottom right: mean SARS-CoV-2 tests performed over 7 sliding days.

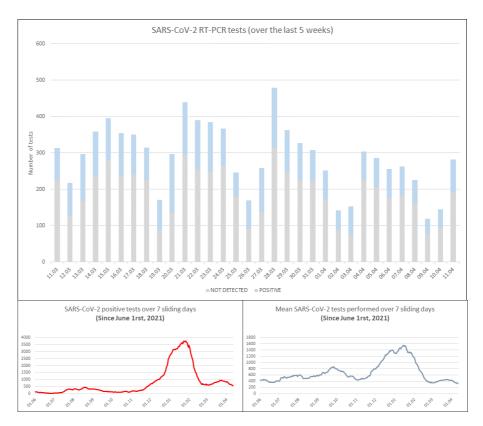


Figure 2: Weekly evolution of the S Drop out among specimens collected at HUG (including both ambulatory and hospitalized patients). Note that because of the high number of positive samples, surveillance was shifted towards hospitalized patients during week 1, and only a random selection of specimens collected at our outpatient department was tested for the S Drop out between week 1 and 7. Since the beginning of week 7 (February 14), all positive samples collected at HUG (both in in- and outpatients) with a Ct value < 32 are tested for the S Drop out. Acknowledgements: S Yerly.


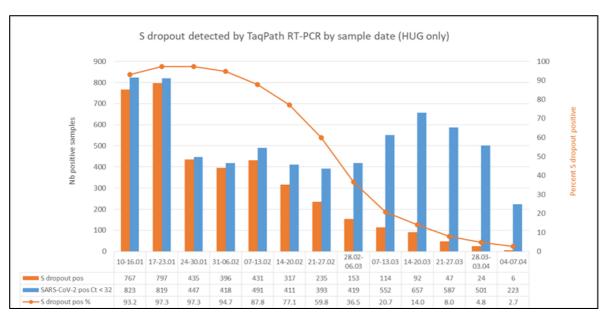


Figure 3: SARS-CoV-2 lineages identified by whole-genome sequencing at HUG from samples (Ct-value \leq 32) collected from Geneva residents (Sentinella specimens excluded). *Sequencing is still ongoing for week 13 (March 28 to April 3, 2022). A total of 889 sequences are included in this analysis.

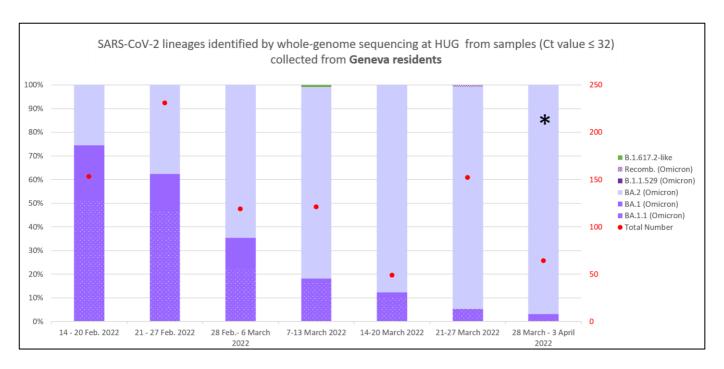

Laurent Kaiser, Samuel Cordey, Manuel Schibler and Pauline Vetter for HUG. Pauline Brindel for the Geneva Cantonal Physician team.

The laboratory of virology of the Geneva University Hospitals as a sentinel site for the Geneva area

The number of tests (PCR and antigen tests) performed at the Geneva University Hospitals represented around 22% (2352/10882) of the total number of tests performed in the canton of Geneva during week 14 of 2022. Roughly 21% of the positive specimens collected in the Geneva area were processed at HUG during this period (580/2788). Samples collected from symptomatic individuals at our outpatient testing center are tested by RT-PCR. Specimens analyzed in our laboratory originate from ambulatory and hospitalized patients as well as symptomatic and/or asymptomatic health care workers.

The number of positive tests in the canton and the total number of tests done during the surveilled week are available on the website from Federal Office of Public Health (COVID-19 Suisse | Coronavirus | Dashboard (admin.ch)). During week 14 in the canton of Geneva, the number of RT-PCR tests and the number of positive cases continued to decrease compared to the previous week. The proportion of positive tests also shows the first signs of decline. However, we continue to observe a high positivity rate above 30% in the Canton of Geneva.

Methods and collaborations

On November 28 2021, screening for the "S drop out" was implemented at HUG on SARS-CoV-2 positive specimens with a Ct-value ≤ 32 that were tested for primary diagnosis in our laboratory (Taqpath RT-PCR assay). The "S drop out" corresponds to the S-gene PCR target not being amplified("dropping out"), while the two other PCR targets are still detected, and serves as a proxy for Omicron BA.1.

All positive specimens were tested for the S drop out between December 1 and 31, 2021. Since January 2022, all specimens originating from hospitalized patients and a selection of specimens collected from ambulatory patients are tested for the "S Drop out". With the decrease in the number of new cases since the beginning of week 7 (February 14), all positive samples collected at HUG (both in in- and outpatients) with a Ct value < 32 and processed at our laboratory are tested for the S Drop out.

Whole genome sequencing performed on SARS-CoV-2 positive samples allows for definitive sublineage/variant identification.

WGS is carried out in close collaboration with the Health 2030 Genome Center in Geneva and Philippe Le Mercier from the Swiss Institute of Bioinformatics. Since March 1, 2021, the sequencing has been done within the Swiss national SARS-CoV-2 genomic and variants surveillance program. Specimens collected at HUG with a Ct-value ≤32 are sequenced. In some instances, sequencing can be done on specimens sent by other laboratories in Switzerland within the surveillance program or by request of the cantonal physician team. Phylogenetic analysis data are produced by Nextstrain, in collaboration with Richard Neher's group at the University of Basel. In addition, partial Sanger sequencing may be done by our laboratory.

Geographic distribution, transmission advantage estimates and detailed numbers of available sequences over time in the canton of Geneva are available on the covSPECTRUM platform, run by Tanja Stadler's group at ETH Zurich.

These reports are produced in collaboration with the Geneva Cantonal Physician team, which provides information on epidemiological links. For epidemiological data, please refer to the weekly report of the cantonal physician team.